










1.4-2.6 TM
PULL THRU
FEEL THE CLEAN

Single Patient Use Channel Cleaning Brush



1.4 - 2.6 mm id

≈ 750-2500 mm


 Single use only
 USE WET
 Read instructions before use
 NON STERILE









see www.pullthru.net.nz for more information











 F R Galantai Manufacturing Co. Ltd
 11 Bancroft Crescent, Glendene
 Auckland, 0602
 New Zealand
 ISO 13485:2016 Certified Site

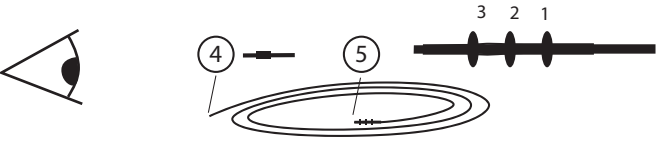New Zealand Patent Number 540125,
 Other International Patents Pending
 Copyright © 2018 F R Galantai Manufacturing Co.Ltd.
 Trademarks are the property of their respective owners


 Advena Ltd.
 Tower Business Centre, 2nd Flr.,
 Tower Street, Swatar,
 BKR 4013 Malta






 X Y

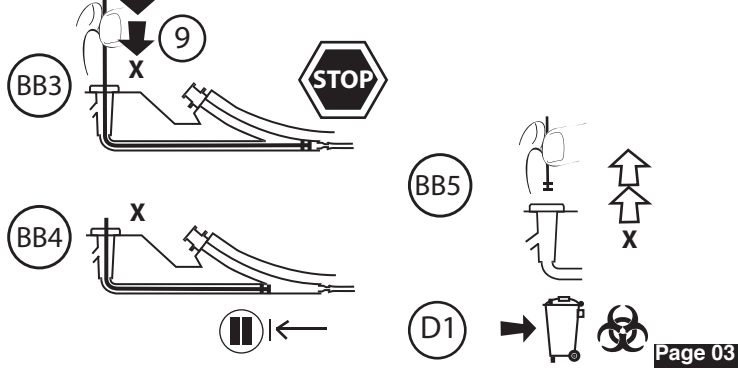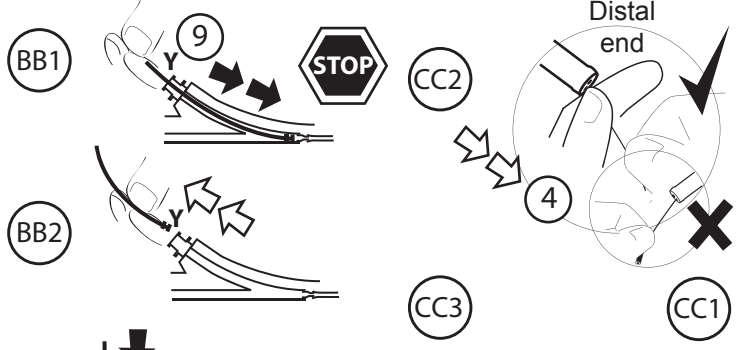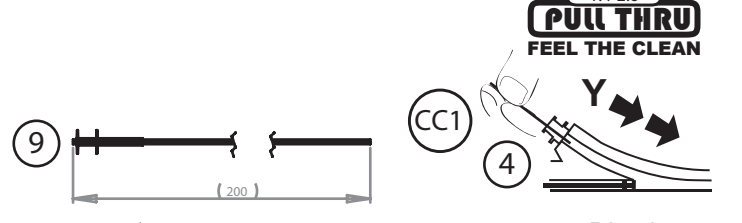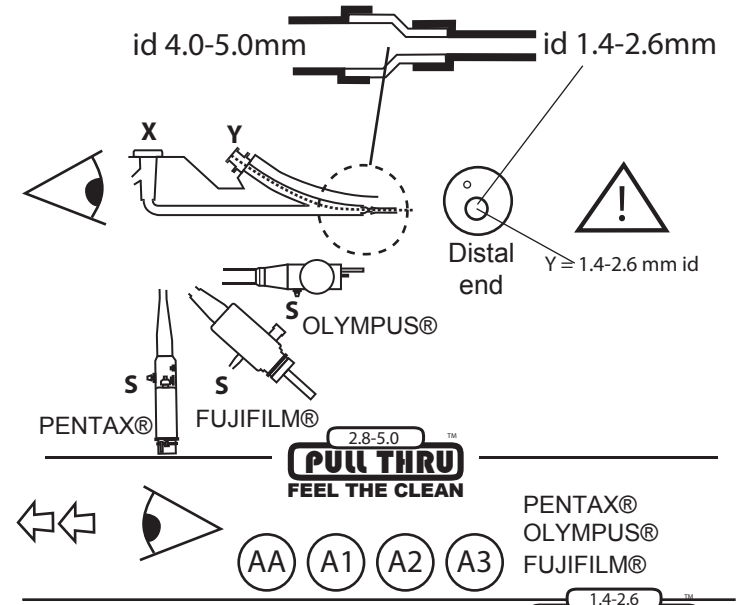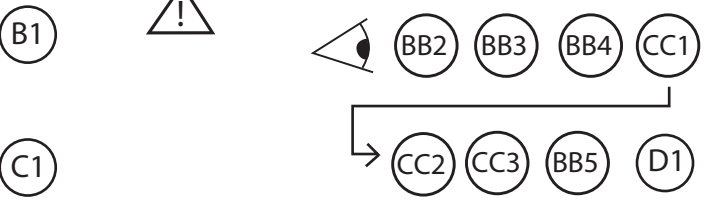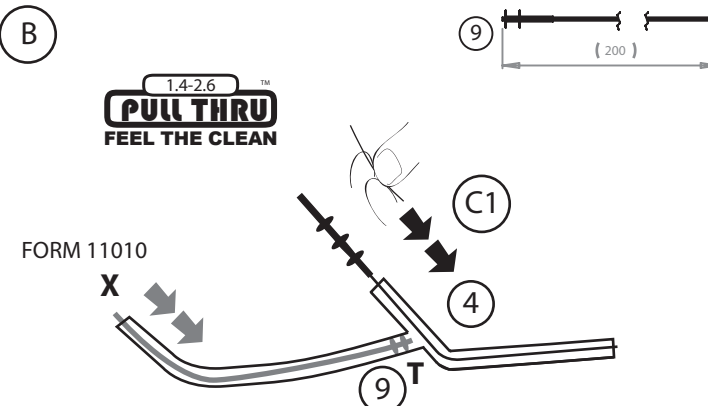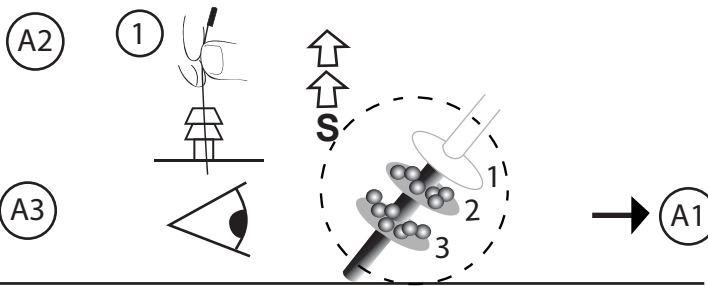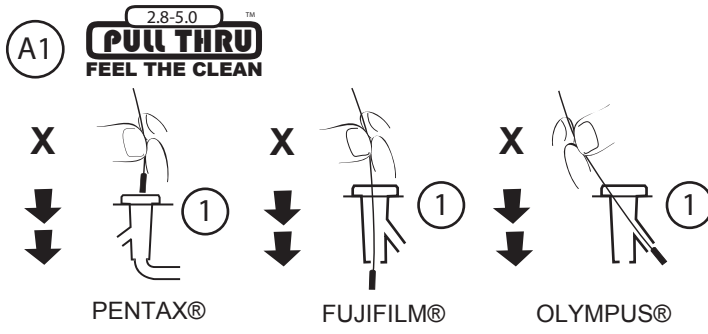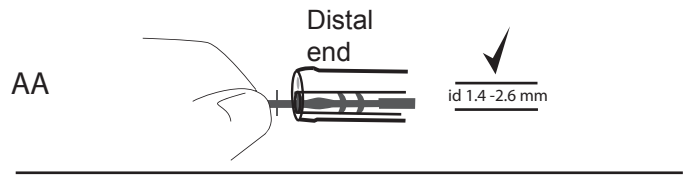 PENTAX® FUJIFILM®
 Distal end
 Y = 2.8-5.0 mm id

FORM 5010
 FORM 4010 Rev 16 May 2020

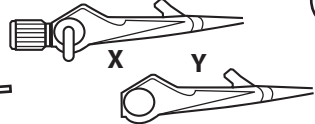



OLYMPUS®

X Y






PUSH THRU
FEEL THE CLEAN
FORM 11010

PULL THRU
FEEL THE CLEAN
1.4-2.6


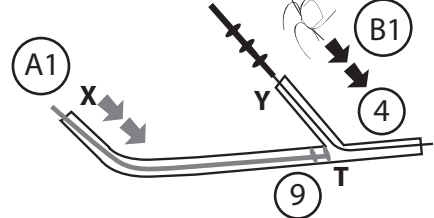


PENTAX®



PUSH THRU
FEEL THE CLEAN
FORM 1101x

PULL THRU
FEEL THE CLEAN
1.4-2.6

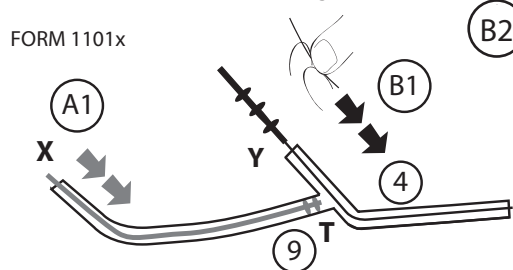


PUSH THRU
FEEL THE CLEAN

PULL THRU
FEEL THE CLEAN

Page 03 BB3 BB4 CC1

CC2 CC3 BB5 D1

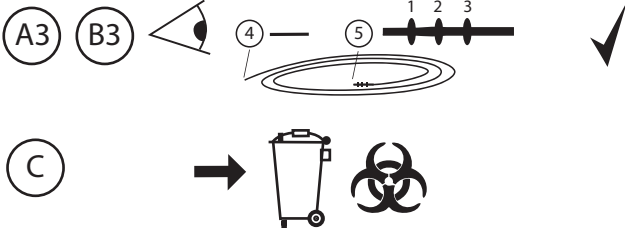

C



STUBBY BRUSH

Single Patient Use Channel Cleaning Brush



Single use only











USE WET



Read Instructions before use



NON STERILE

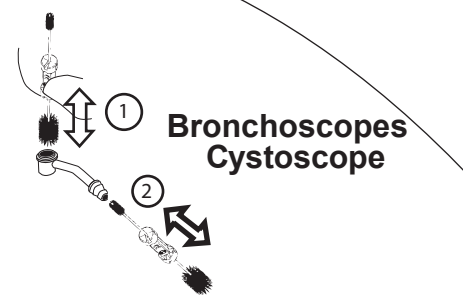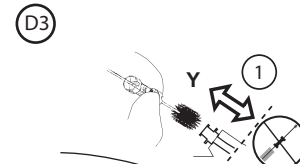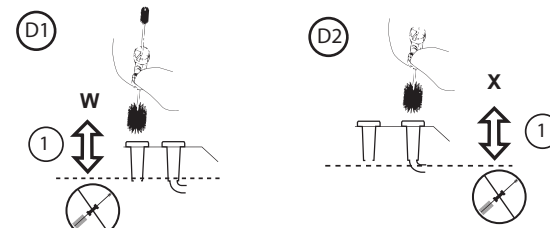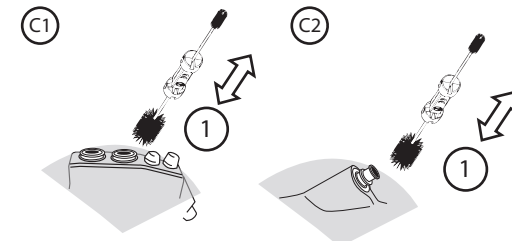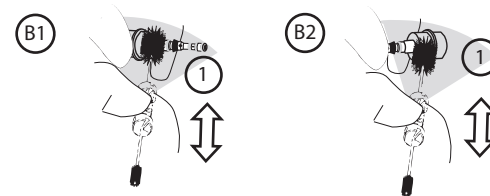

Bronchoscope Cystoscope

